



Fabrication of pedestal high-contrast grating for biosensing applications

Beliaev, Leonid Yu.; Stounbjerg, Peter Groth; Finco, Giovanni; Bunea, Ada-loana; Malureanu, Radu; Lindvold, Lars René; Takayama, Osamu; Andersen, Peter E.; Lavrinenko, Andrei V.

Publication date:
2022

Document Version
Publisher's PDF, also known as Version of record

[Link back to DTU Orbit](#)

Citation (APA):
Beliaev, L. Y., Stounbjerg, P. G., Finco, G., Bunea, A-I., Malureanu, R., Lindvold, L. R., Takayama, O., Andersen, P. E., & Lavrinenko, A. V. (2022). *Fabrication of pedestal high-contrast grating for biosensing applications*. Abstract from 48th International Conference on Micro and Nano Engineering, Leuven, Belgium.

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

Fabrication of pedestal high-contrast grating for biosensing applications

Leonid Yu. Beliaev ^a, Peter Groth Stounbjerg ^b, Giovanni Finco ^{a,c}, Ada-Ioana Bunea ^d, Radu Malureanu ^a, Lars René Lindvold ^b, Osamu Takayama ^a, Peter E. Andersen ^b, and Andrei V. Lavrinenko ^a

^a DTU Fotonik – Department of Photonics Engineering, Technical University of Denmark, Ørstedes Plads, Building 345A, DK-2800 Kongens Lyngby, Denmark.

^b DTU Health Tech – Department of Health Technology, Technical University of Denmark, Ørstedes Plads, Building 345C, DK-2800 Kongens Lyngby, Denmark.

^c Optical Nanomaterial Group, Institute for Quantum Electronics, Department of Physics, ETH Zürich, Auguste-Piccard-Hof 1, HPT D5, 8093 Zürich, Switzerland.

^d DTU Nanolab - National Centre for Nano Fabrication and Characterization, Technical University of Denmark, Ørstedes Plads, Building 347, DK-2800 Kongens Lyngby, Denmark.

e-mail: adabu@dtu.dk

Many different approaches and detection principles are used for optical biosensing [1-5]. One example is refractometric sensing, where the analyte is detected because its presence causes changes in the local refractive index, which in turn leads to a shift of the resonance position. High-contrast grating (HCG) structures can be employed in refractometric sensing due to their narrow resonance and high sensitivity [6,7].

Here, we present the fabrication and characterization of pedestal-HCG structures, which were chosen as promising candidates for improved biosensing based on theoretical calculations [7]. Moreover, we show an experimental comparison of their performance with conventional HCG. The structures were optically characterized in terms of both bulk and surface sensing.

The fabrication process comprises deep UV lithography for defining the pattern and dry etching for generating the final structures. All fabrication steps are depicted in Fig. 1(a). First, the home-made silicon-on-insulator (SOI) substrates were prepared by a wet oxidation process based on H₂O at 1100 °C, resulting in a 1.1 μm SiO₂ layer on Si, and a low pressure chemical vapor deposition (LPCVD) step based on SiH₄ at 560 °C, to grow 500 nm of amorphous Si (aSi) on top of the SiO₂ layer. The next step involved a conventional deep-UV lithography process where a one-dimensional periodic lattice of bars (lattice period $\Lambda = 810$ nm and bars width $w = 340$ nm) was introduced onto the aSi surface. Deep reactive ion etching was used afterwards to etch down bars through the aSi layer. For the last step, the HF vapor phase was used for the controllable etching of the SiO₂ layer underneath the aSi grating bars.

To characterize the potential of the structures for biosensing applications, their surface sensitivity and bulk refractive index sensitivity (BRIS) were evaluated from reflection spectra as shown in Fig.2. We deposited on the surface of our structures 2-5 nm thick layers of Al₂O₃ (refractive index (RI) = 1.6) using atomic layer deposition. The resonance position shift, which is determined by the deposited oxide thickness, is 10.5% more apparent for pedestal-HCG than for conventional HCG. In terms of BRIS, the performance of pedestal HCG is 11.2% higher than that of the conventional HCG (536 nm/RIU (refractive index unit) as opposed to 482 nm/RIU). This experimental performance increase confirms the theoretical predictions from [7].

To sum up, the performance of pedestal-HCG in terms of surface and bulk sensitivity surpasses that of conventional HCG, suggesting that the pedestal-HCG are good candidates for biosensing applications.

- [1] X. Fan et al, *Anal. Chim. Acta* 620, 8–26 (2008).
- [2] G. Pitruzzello et al, *J. Opt.* 20, 1–23 (2018).
- [3] F. Yesilkoy et al, *Nature Photon.* 13, 390–396 (2019).
- [4] E. Shkondin et al, *Opt. Mater. Express* 7, 4171–4182 (2017).
- [5] L. Yu. Beliaev et al, *Opt-Electron. Adv.* 4, 1–27 (2021).
- [6] T. Sun et al, *Sci. Rep.* 6, 27482 (2016).
- [7] G. Finco et al, *Nanophotonics* 10, 4289–4296 (2021).

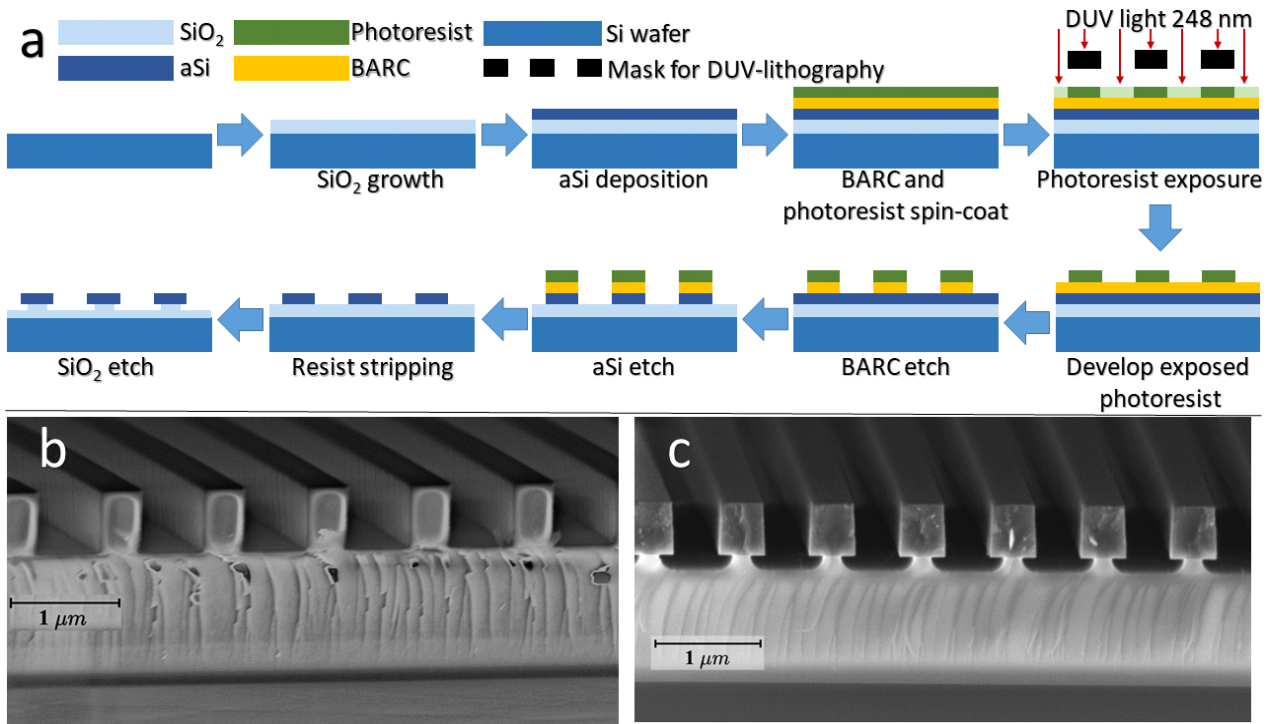


Figure 1. (a) Schematic of the fabrication process for the pedestal high-contrast grating. (b) SEM image of the HCG in cross-section, (c) SEM image of the pedestal-HCG in cross-section.

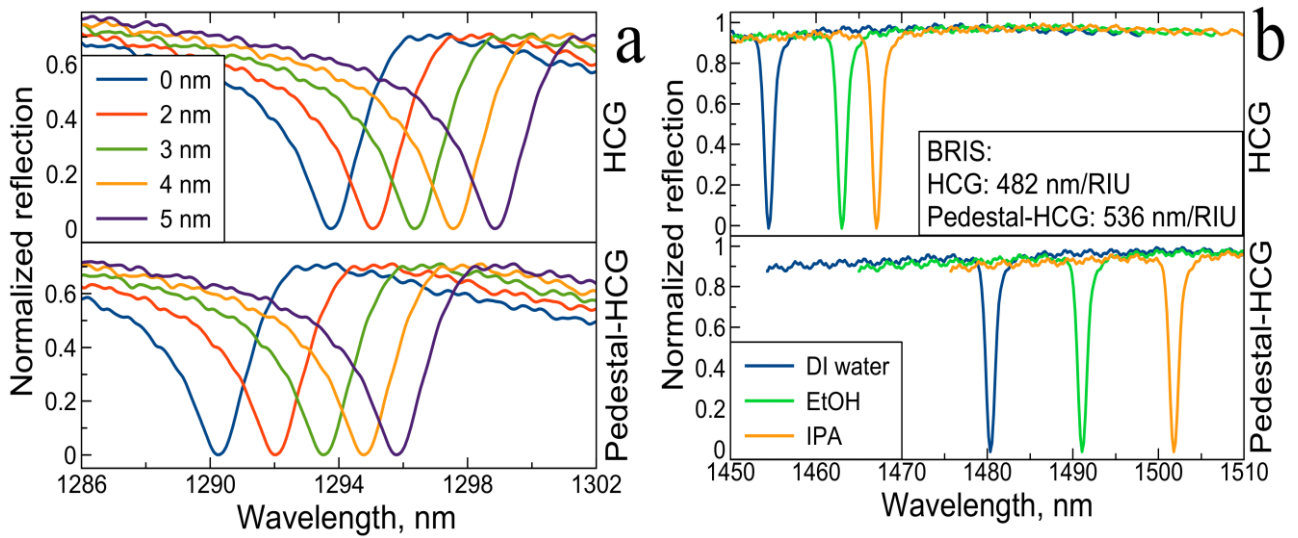


Figure 2. (a) Reflection spectra of conventional and pedestal high contrast gratings measured with different deposited thicknesses of Al_2O_3 . (b) Reflection spectra of conventional and pedestal high contrast gratings in deionized water, ethanol and isopropanol media, which have a refractive index of 1.33, 1.35 and 1.37, respectively.