



A Validated Template for Computational Dose Modelling for Transcranial Focused Ultrasound Stimulation

Hosseini, Seyed sina; Puonti, Oula; Treeby, Bradley; Hanson, Lars G. ; Thielscher, Axel

Publication date:
2022

Document Version
Peer reviewed version

[Link back to DTU Orbit](#)

Citation (APA):

Hosseini, S., Puonti, O., Treeby, B., Hanson, L. G., & Thielscher, A. (2022). *A Validated Template for Computational Dose Modelling for Transcranial Focused Ultrasound Stimulation*. Abstract from 3rd Focused Ultrasound Neuromodulation, Mainz, Rhineland-Palatinate, Germany.

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

Title: A Validated Template for Computational Dose Modelling for Transcranial Focused Ultrasound Stimulation

Authors: Seyedsina Hosseini^{1,2}, Oula Puonti², Bradley Treeby³, Lars G. Hanson^{1,2}, Axel Thielscher^{1,2}
1 Department of Health Technology, Technical University of Denmark, Kgs. Lyngby, Denmark
2 Danish Research Centre for Magnetic Resonance, Copenhagen University Hospital Amager and Hvidovre, Denmark
3 Department of Medical Physics and Biomedical Engineering, University College London, Gower Street, London, WC1E 6BT, United Kingdom

Email: seyho@dtu.dk

Abstract:


Background: Transcranial focused ultrasound stimulation (TUS) is emerging as a novel non-invasive method with far better spatial resolution than existing non-invasive brain stimulation methods and the unique ability to create small stimulation foci in deep brain areas. However, accurate focusing of the TUS acoustic waves through the intact human skull is problematic as the skull causes strong attenuation and reflection of the waves. As in-vivo acoustic wave measurements are not yet feasible, computer simulations are required to determine the spatial distribution and intensity of the acoustic wave after skull transmission.

Methods: Our work focuses on establishing accurate computer simulations of the TUS acoustic wave based on information of the skull morphology and its acoustic properties estimated from computed tomography (CT) images. As it is often challenging to obtain high-quality imaging data for individual participants, we are currently working on establishing a skull template that can be used to estimate the average effects of the skull on the TUS acoustic wave in the population. A reliable skull template can also provide valuable information as part of the study development process, including investigating different transducer alignment strategies, acoustic distortions, and safety metrics. The template was made from CT and magnetic resonance images (MRI) of the heads of thirty individuals of different ages (between 20-50 years old), gender, and ethnicity, using the ANTs [1] registration tool. Additionally, the individual scans were segmented using the CHARM [2] segmentation tool to create masks for skull, internal air cavities, and intracranial tissues. Then, by using the masks and the CT intensity information, a mapping to the acoustic properties was applied [3]. For the next step, the k-Wave [4] toolbox was employed for modeling the acoustic wave distribution for the template and each individual subject. For simulations, a 500 kHz ultrasonic transducer was modeled with a similar size to an existing commercial transducer. For positioning the transducer, 24 different positions based on the 10-20 standard EEG system were used.

Results: To show how well our template represents the population average, we compare different parameters to characterize the acoustic wave distribution and intensity and compare these parameters between the subjects and the template for all transducer positions. As shown in figure (a) these parameters include the amplitude of peak pressure, the volume of the focus area, and the angular deviation of the peak pressure location. In figure (b), the violin plot shows the peak pressure amplitude versus the transducer positions for 27 subjects and the template (shown with red dots). Among 27 subjects, the template results located within the interquartile range of violin plots for 12, 20, and 14 transducer positions out of 24 positions for peak pressure amplitude, FWHM volume, and angular deviation respectively. The results for all thirty subjects will be presented as part of our future work.

Discussion: As shown in figure (b), for some transducer positions, the template represents the average pressure very well, but is less accurate for others. The reason could be due to differences in skull morphology and composition between the template and subjects, which we will investigate further as part of our future work.

[1] Avants, Brian B., et al. *Neuroimage* 54.3 (2011): 2033-2044; [2] Puonti, Oula, et al. *Neuroimage* 219 (2020): 117044; [3] Montanaro H, et al. *Journal of Neural Engineering*. 2021 May 4;18(4):046041; [4] B. E. Treeby, et al. *J. Biomed. Opt.*, vol. 15, no. 2, p. 021314, 2010.

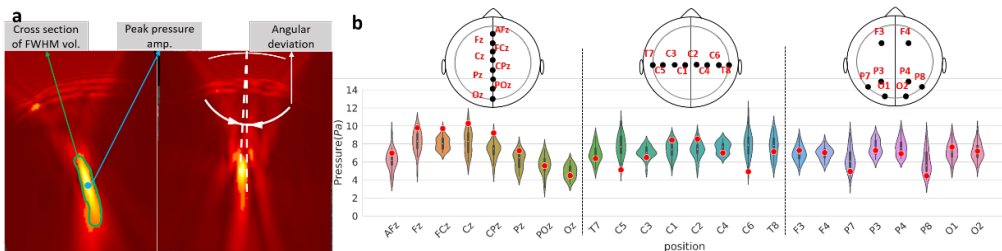

Acknowledgments: This study was supported by the Lundbeck foundation (grant R313-2019-622 to AT)

Conflicts of interest: none

Topic area: technical **Preferred format:** oral

Are you an early career researcher? (trainee, student, post-doc, etc)