



## Upgrade and extension of the climate station at DTU Byg

Andersen, Elsa; Dragsted, Janne; Kristensen, Troels V.; Andersen, Lars Kokholm

*Publication date:*  
2014

*Document Version*  
Publisher's PDF, also known as Version of record

[Link back to DTU Orbit](#)

*Citation (APA):*  
Andersen, E., Dragsted, J., Kristensen, T. V., & Andersen, L. K. (2014). *Upgrade and extension of the climate station at DTU Byg*. Technical University of Denmark, Department of Civil Engineering.

---

### General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

# Upgrade and Extension of the Climate station at DTU Byg



Elsa Andersen  
Janne Dragsted  
Troels V. Kristensen  
Lars Kokholm Andersen

## Technical Report

Department of Civil Engineering  
2014

DTU Civil Engineering Report SR 14-01 (UK)  
July 2014

## Table of Contents

|  |    |
|--|----|
| 1. Preface.....                                  | 1  |
| 2. Background and objective of the project ..... | 2  |
| 3. The new Climate station .....                 | 4  |
| 4. Results from the new Climate station .....    | 11 |
| 5. References .....                              | 14 |

### 1. Preface

In the period 2013-2014 the project “Upgrade and Extension of the Climate Station at DTU Byg” is carried out at DTU Byg. The aim of the project is to renew the hardware and the software for data acquisition and monitoring, exchange cables and cable connections in order to avoid interference of electrical noise from the surroundings and exchange worn out equipment. Further, the aim is to make measured data from the climate station easily available for the users.

The project is financed by the Bjarne Saxhof foundation.

## 2. Background and objective of the project

Detailed measurements of weather data are used to study the weather and develop solar radiation processing models that are needed in order to simulate the energy consumption of buildings, the indoor climate, the thermal performance of solar heating systems and the performance of PV systems. The weather varies from one year to another. Therefore design reference years based on minimum 10 years of measured weather data are used in simulations. In order to work out reliable design reference years, it is needed to know the short term variations in the solar radiation. Hourly values of solar radiation are not always sufficient because of the short time constant of e.g. PV panels. On this background, a solar radiation measurement station was established on the roof of building 119 at DTU Byg. The station was put in operation in 1989 and has been in operation ever since [1], see Figure 1.

The measurements are unique because of the very detailed measurements of the solar radiation, especially the diffuse solar radiation and because of the long measurement period of about 25 years.



Figure 1. Pictures of the solar radiation measurement station before upgrade and renovation. Top left: Measurement equipment. Top middle: Shadow ring. Top right: the old tracker (Eppley). Bottom left: Pyranometer, type CMP 11 from Kipp and Zonen. Bottom middle left: Sunshine pyranometer, type SPN1. Bottom middle right: Weather station, type Vaisala WTX520 from Oyj in Finland. Bottom right: Vaisala mounted 6 meter above the roof of building 119.

The measured weather data from the solar radiation measurement station comprise:

- Global radiation

- Diffuse radiation measured with a shadow ring. The measurements must be corrected afterwards in order to include the part of the diffuse radiation screened of by the shadow ring. The dimensions of the shadow ring are: diameter of 650 mm, width of 58 mm.
- Diffuse radiation measured with a tracker (Eppley) with a disk that screens of the beam radiation from the sun disk. The width of the disk is 5.7°.
- Direct normal beam radiation measured with a pyrheliometer.
- Total solar radiation on 45° tilted south oriented surface
- Total solar radiation on 90° tilted surfaces pointing towards south, east, west and north
- Long wave radiation to the sky
- Ambient temperature
- Relative humidity
- Dew point temperature

The tracker (Eppley) was modified with a step motor and a control system for the step motor that moved the tracker/changed the azimuth angle of the tracker every 2 minutes. The zenith angle was adjusted manually three times a week. The shadow ring from the other diffuse radiation measurement was adjusted at the same time/frequency as the zenith angle of the tracker.

The data logging was running on a very old DOS based computer without internet connection and today it is no longer possible to get service and spare parts for the old computer.

In 2008 a Vaisala weather station was added to the solar radiation measurement station. The Vaisala weather station was positioned 6 meters over the roof and added measurements of rain (rainfall, rain current and peak intensity, duration of a rain event), wind speed and wind direction, atmospheric pressure, ambient temperature and humidity to the test facility.

The solar radiation measurement station was renamed to Climate station.

The measurements are frequently used in research projects and in student projects and it is considered to be in the interest of DTU Byg to keep this unique Climate station in operation.

Much manpower has been used in order to keep the test facility in operation since 1989. The work load included adjustment of the shadow ring and the tracker, maintenance of the tracker, cleaning of the instruments, calibrating the instruments and making sure the data was good and useful and servicing the users by supplying the weather data that was asked for. All in all, the load of maintenance, operation and service of users has been very time consuming.

The objective of this project is to renovate and upgrade the Climate station to the standard of today in order to minimize the work load related to operating the Climate station and providing service to the users.

### 3. The new Climate station

The new Climate station has got new hardware and new software. The hardware is from National Instruments and comprises a compactRIO control and monitoring system with a number of input/output modules, I/O modules. The compactRIO is a stand-alone computer with internet access. In case of a power failure, the compactRIO will automatically restart when the power is back. The I/O modules are analogue input modules of the types NI9205 and NI9214 that both measure the voltage from the pyranometers and type NI9217 that measures the temperatures from PT100 sensors. Apart from two RS232 channels on the compactRIO, the monitoring system has one RS232 module, type NI9870 with four channels. The RS232 channels allow the readings from the sunshine pyranometer, type SPN1 and the readings from the Vaisala weather station, type WXT520 from Oyj in Finland to be included in the measurement program, see figure 2.

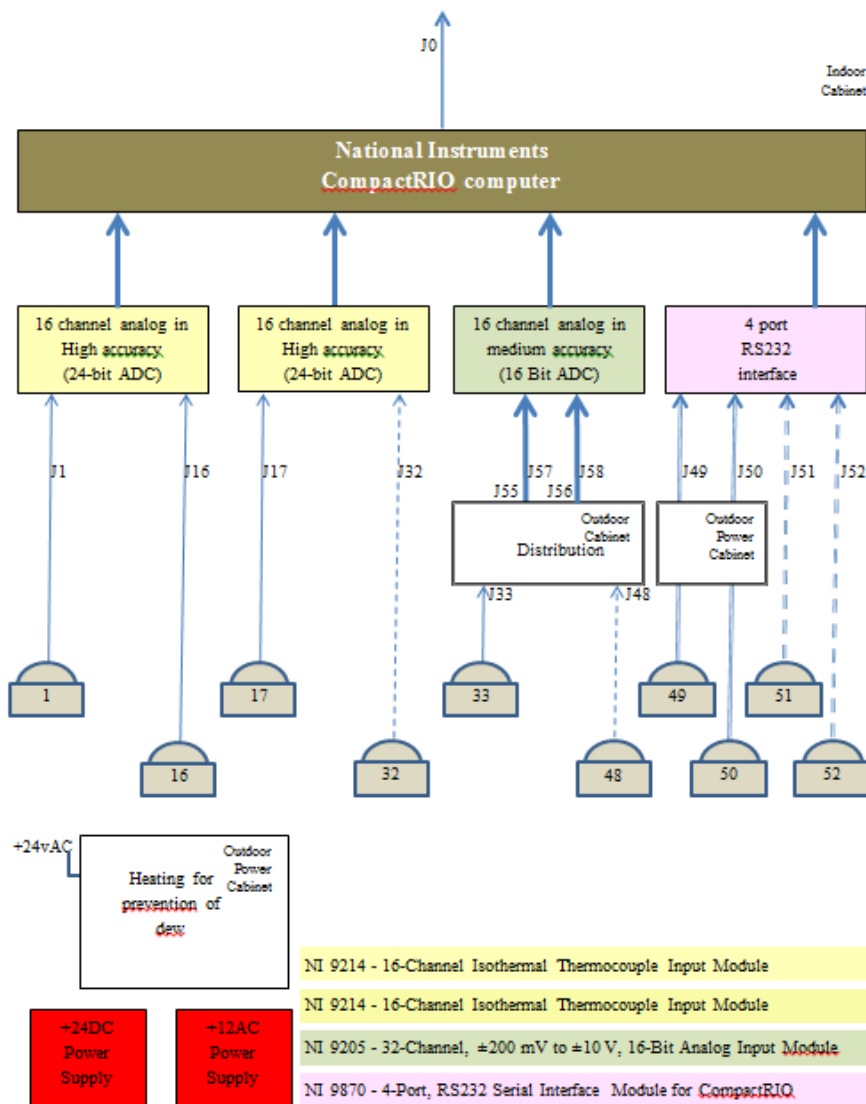


Figure 2. Schematically illustration of the data acquisition and monitoring setup and the cable connections between the instruments and the data monitoring system.

Also, new 230 Volt AC power installation is established at the climate station. This installation supplies the power to the tracker and to small heating loops used to evaporate moisture from the glass domes of the pyranometers, see figure 3 and figure 4.

To eliminate dew, heating elements are mounted around the glass dome:

- heating element made of copper-constantan thermo couple type TT. 2.75 m TT winded as a long spiral. The element emits 10 W of heat at 12 Vac.

The power supply is a dual output 12 Vac transformer and can support a maximum of 40 Heat elements.

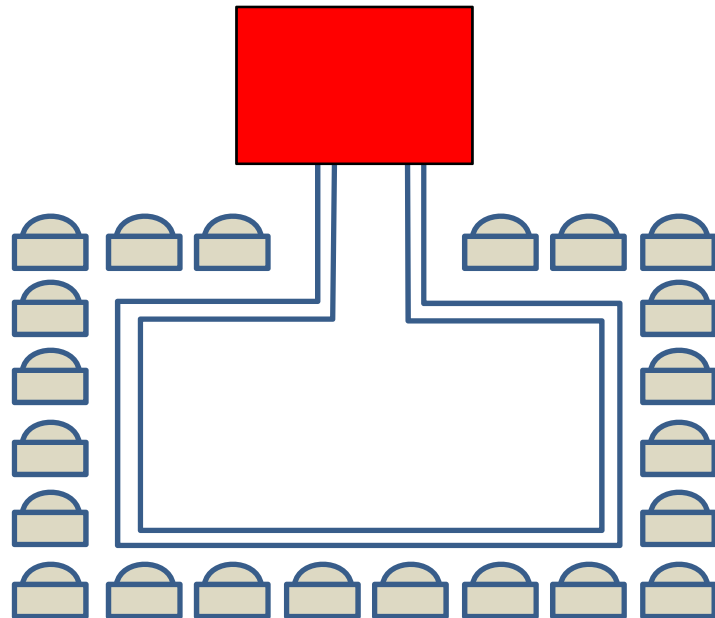


Figure 3. 12 Vac power supply.



Figure 4. Pictures of the heating elements used to evaporate moisture from the glass dome of pyranometers.

In order to eliminate noise from electrical sources in the surroundings of the cables from the instruments to the data logger, the cables are twisted pairs with 80% braid coverage. The data logger is placed in an Electromagnetic Compatibility, EMC cabinet. Another EMC cabinet is placed

outdoor at the platform of the Climate station. All connections are carried out with shielded plugs. In this way electrical noise cannot disturb the measurements, see figure 5.

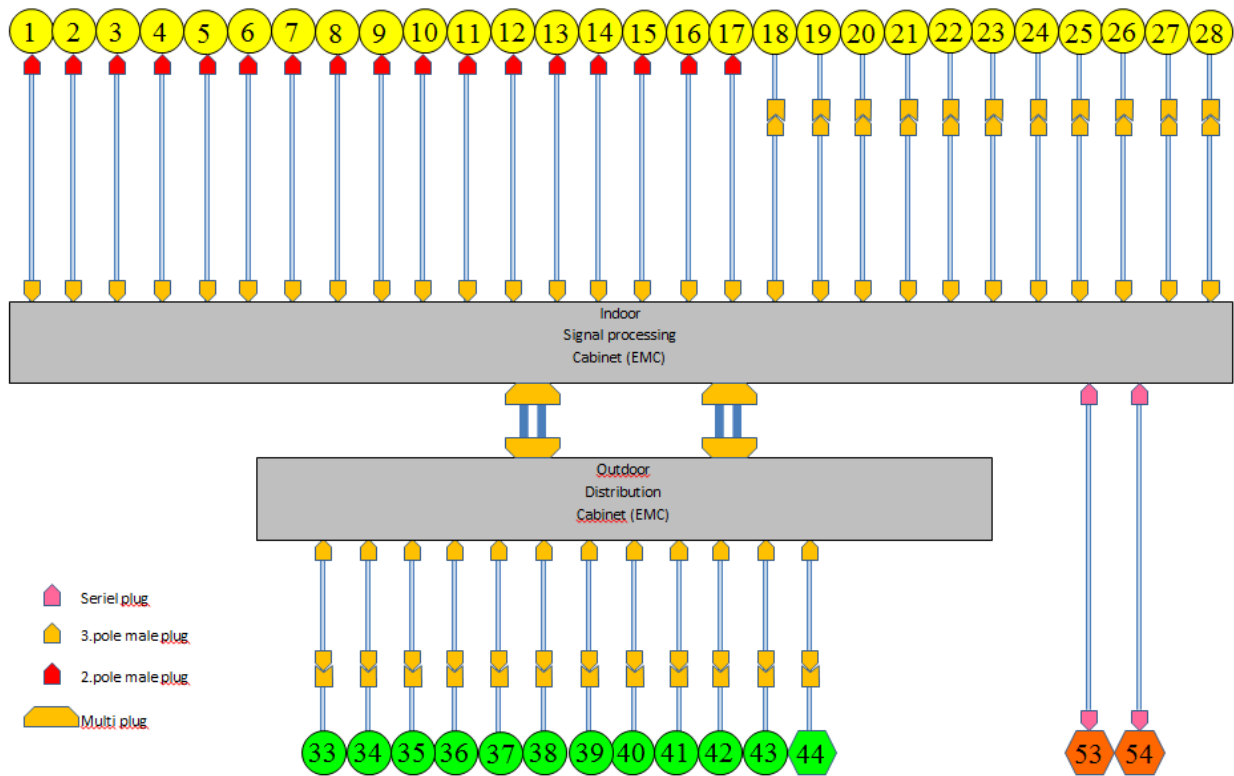


Figure 5. Connector types.

With one NI9205 I/O module and two NI9214 I/O modules, it is possible to measure the response from 48 different solar radiation instruments. The measurement accuracy of NI9205 lays in the range 11 – 55  $\mu\text{V}$  corresponding to an accuracy in the range 1.5 – 10  $\text{W}/\text{m}^2$  while the accuracy of NI9214 is about 8  $\mu\text{V}$  corresponding to an accuracy of around 1  $\text{W}/\text{m}^2$ .

The old tracker has been replaced by a new tracker from Kipp and Zonen, type SOLYS 2. This tracker has an integrated GPS receiver that allows the tracker to automatically determine its location and the time and operate according to this. Apart from this the tracker has been equipped with a solar sensor from Kipp and Zonen for active tracking. The solar sensor fine tunes the tracking perfectly.

A pyranometer from Kipp and Zonen, type CMP 11 for measuring of the diffuse radiation and a pyrhelimeter, type CHP 1 for measuring of the beam normal radiation are mounted on the tracker, see figure 6.





Figure 6. The SOLYS 2 tracker. On the top mounting plate, the pyranometer that measures the diffuse irradiance can be seen. On the left side of the tracker, the solar sensor and the pyrheliometer that measured the beam normal irradiance can be seen.

Apart from the new measurement equipment, most of the old measurement equipment is renovated and reused. Table 1 shows the measurement equipment in operation at the climate station. Figure 7 shows a top view of the climate station with indication of the location of the different measurement instruments. The colors distinguish between how the instruments are connected to the data logger according to figure 5.

By means of the pyranometers inside the domes numbered 1-16 it is possible to determine diffuse radiation from different parts the sky [2].

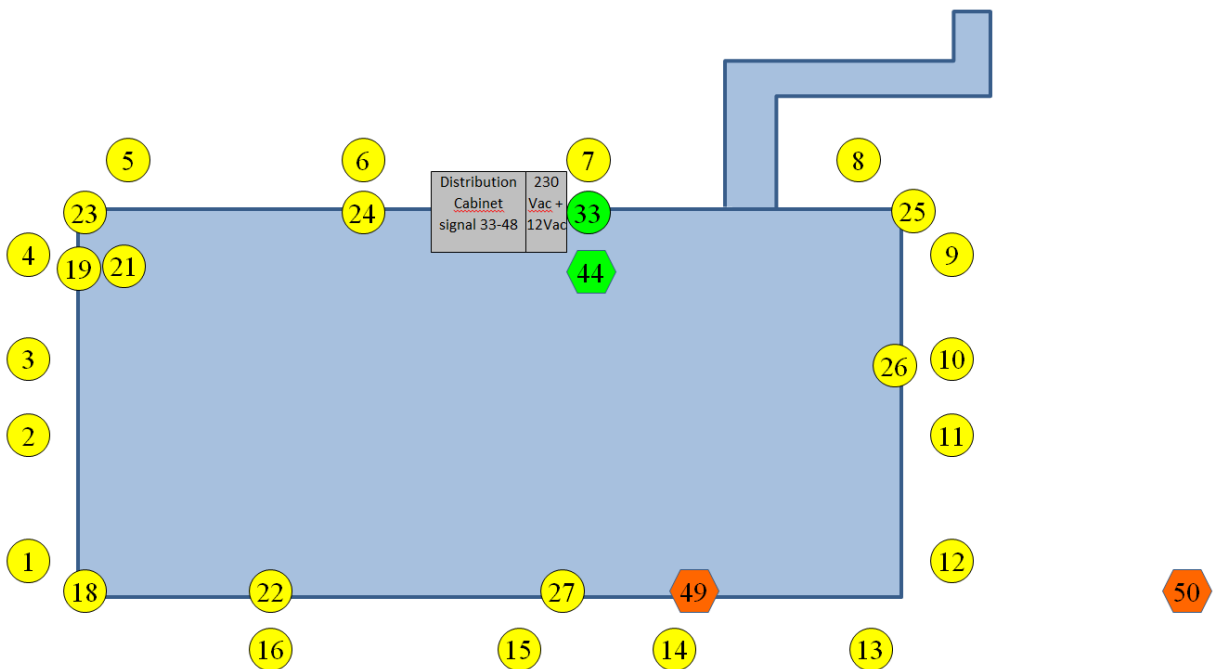


Figure 7. Top view of the Climate station with numbering and placement of the instruments. The numbers correspond to the numbers in table 1.

Table 1. Measurement equipment in use at the new Climate station.

|    | Parameter   | Resolution           | Sensor | Accuracy | Correction |
|----|---|----------------------|--------|----------|------------|
| 1  | Pyranometer. 1/8 Dome. Azimuth=39.5°  | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 2  | Pyranometer. 1/16 Dome. Azimuth=39.5°   | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 3  | Pyranometer. 1/8 Dome. Azimuth=84.5°  | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 4  | Pyranometer. 1/16 Dome. Azimuth=84.5°   | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 5  | Pyranometer. 1/8 Dome. Azimuth=129.5°   | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 6  | Pyranometer. 1/16 Dome. Azimuth=129.5°  | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 7  | Pyranometer. 1/8 Dome. Azimuth=174.5°   | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 8  | Pyranometer. 1/16 Dome. Azimuth=174.5°  | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 9  | Pyranometer. 1/8 Dome. Azimuth=-140.5°  | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 10 | Pyranometer. 1/16 Dome. Azimuth=-140.5°   | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 11 | Pyranometer. 1/8 Dome. Azimuth=-95.5°   | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 12 | Pyranometer. 1/16 Dome. Azimuth=-95.5°  | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 13 | Pyranometer. 1/8 Dome. Azimuth=-50.5°   | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 14 | Pyranometer. 1/16 Dome. Azimuth=-50.5°  | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 15 | Pyranometer. 1/8 Dome. Azimuth=-5.5°  | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 16 | Pyranometer. 1/16 Dome. Azimuth=-5.5°   | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 17 | Not in use  |                      |        |          |            |
| 18 | Pyranometer for diffuse irradiance on horizontal measured with shadow ring: Radius=650 mm. Width=58 mm.                             | 0.1 W/m <sup>2</sup> | CM11   | 1.4 %    | Needed     |
| 19 | Pyranometer for diffuse irradiance on horizontal measured with tracker.   | 0.1 W/m <sup>2</sup> | CMP11  | 1.4 %    | see fig. 8 |
| 20 | Not in use  |                      |        |          |            |
| 21 | Pyrheliometer for beam normal irradiance. Internal instrument temperature measured with PT100 (see # 53)                            | 0.1 W/m <sup>2</sup> | CHP1   | 1 %      |            |
| 22 | Pyranometer for global irradiance   | 0.1 W/m <sup>2</sup> | CM11   | 1.4 %    | see fig. 8 |
| 23 | Pyranometer for total solar irradiance on 90° tilt West oriented  | 0.1 W/m <sup>2</sup> | CM5    | 3 %      |            |
| 24 | Pyranometer for total solar irradiance on 90° tilt North oriented   | 0.1 W/m <sup>2</sup> | CM5    | 3 %      |            |
| 25 | Pyranometer for total solar irradiance on 90° tilt East oriented. Artificial horizon for rejection of ground reflected irradiance.  | 0.1 W/m <sup>2</sup> | CM5    | 3 %      |            |
| 26 | Pyranometer for total solar irradiance on 90° tilt South oriented. Artificial horizon for rejection of ground reflected irradiance. | 0.1 W/m <sup>2</sup> | CM11   | 1.4 %    | see fig. 8 |
| 27 | Pyranometer for total solar irradiance on 45° tilt South oriented.  | 0.1 W/m <sup>2</sup> | CM5    | 3 %      | see fig. 8 |
| 28 |   |                      |        |          |            |
| 29 |   |                      |        |          |            |
| 30 |   |                      |        |          |            |
| 31 |   |                      |        |          |            |
| 32 |   |                      |        |          |            |
| 33 | Pyrgeometer. Atmospheric infrared   | 0.1 W                | CGR 3  | 5 %      |            |

|    |   |                    |  |               |  |
|----|---|--------------------|--|---------------|--|
|    | radiation (PIR).  |                    |  |               |  |
| 34 |   |                    |  |               |  |
| 35 |   |                    |  |               |  |
| 36 |   |                    |  |               |  |
| 37 |   |                    |  |               |  |
| 38 |   |                    |  |               |  |
| 39 |   |                    |  |               |  |
| 40 |   |                    |  |               |  |
| 41 |   |                    |  |               |  |
| 42 |   |                    |  |               |  |
| 43 |   |                    |  |               |  |
| 44 | Old weather station placed under the solar radiation measurement platform.<br>Temperature / relative humidity   | 0.01 °C /<br>0.5 % | Vaisala<br>HMP45<br>A,<br>PT1000<br>/<br>DOL<br>14 | 0.2 % /<br>?? |  |
| 45 |   |                    |  |               |  |
| 46 |   |                    |  |               |  |
| 47 |   |                    |  |               |  |
| 48 |   |                    |  |               |  |
| 49 | Sunshine pyranometer. SPN1, see table 2   |                    |  |               |  |
| 50 | Vaisala weather station, see table 3  |                    |  |               |  |
| 51 | Not in use  |                    |  |               |  |
| 52 | Not in use  |                    |  |               |  |
| 53 | Pyrheliometer instrument internal temperature (see #21)<br>Should be used for temperature compensation: Temperature [°C] ; diviation [%]: 50 40 30 20 10 0 -10 -20 ; 0.16 -0.02 -0.07 0.00 0.18 0.19 0.05 -0.48 |                    | RTD0_<br>pyrheliometer                             |               |  |
| 54 | Not in use  |                    | RTD1   |               |  |
| 55 | Not in use  |                    | RTD2   |               |  |
| 56 | Indoor Cabinet internal temperature   |                    | RTD3   |               |  |

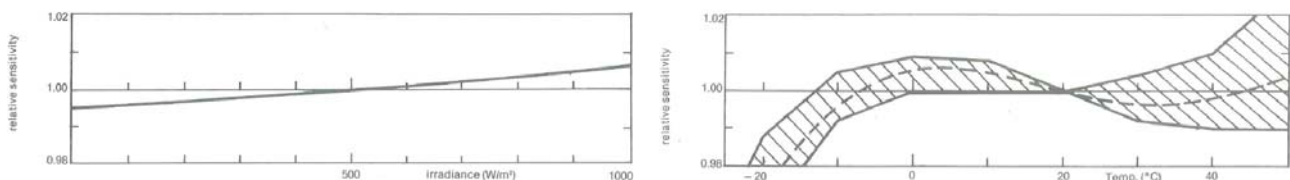


Figure 8. Left: Sensitivity variation with irradiance of Kipp & Zonen pyranometer CM 11 and CMP 11. Right: Relative sensitivity variation with instrument temperature of CM 11 and CMP 11 when placed in a shaded region.

Table 2. Output from the sunshine pyranometer SPN1.

| 49 | Parameter                      | Resolution     |   |
|----|--------------------------------|----------------|---|
|    | Sunshine                       | 0 / 1          | 0 if solar irradiance $\leq 300 \text{ W/m}^2$<br>1 if solar irradiance $> 300 \text{ W/m}^2$ |
|    | sun_total [ $\text{W/m}^2$ ]   | $\text{W/m}^2$ |   |
|    | sun_diffuse [ $\text{W/m}^2$ ] | $\text{W/m}^2$ |   |

Table 3. Output from the Vaisala weather station.

| 50 | Parameter  | Resolution                |   |
|----|--|---------------------------|---|
|    | wind_speed_min [m/s]<br>wind_speed_avg [m/s]<br>wind_speed_max [m/s] | 0.1 m/s                   | The greater of 0.3 m/s or 3% of the measurement range 0...35 m/s<br>5% for the measurement range of 36...60 m/s   |
|    | wind_dir_min [°]<br>wind_dir_avg [°]<br>wind_dir_max [°]             | 1°                        | 3°  |
|    | air_temperature [°C]   | 0.1 °C                    | 0.3 °C at ambient temperature of 20 °C. For accuracy over temperature range, see figure 9   |
|    | relative_humidity [%]  | 0.1 %RH                   | 3 %RH at 0...90 %RH<br>5 %RH at 90...100 %RH  |
|    | air_pressure [Pa]  | 10 Pa                     | 0.5 hPa at ambient temperature range 0...36 °C<br>1 hPa at ambient temperature range -52...60 °C  |
|    | rain_fall [mm]   | 0.01 mm                   | Cumulative accumulation after latest auto reset.<br><br>5 %, weather dependent. Due to the nature of the phenomenon, deviations caused by spatial variations may exist in precipitation readings, especially in short time scale. The accuracy specification does not include possible wind induced error |
|    | rain_duration [s]  | 10 s                      | Counting each 10-second increment whenever droplets detected.   |
|    | rain_intensity [mm/h]  |                           | Running one minute average in 10-second steps   |
|    | Hail [hits/cm <sup>2</sup> ]   | 0.1 hits/cm <sup>2</sup>  | Cumulative amount of hits against collecting surface.   |
|    | hail_duration [s]  | 10 s                      | Counting each 10-second increment whenever hailstone detected.  |
|    | hail_intensity [hits/cm <sup>2</sup> h]                              | 10 hits/cm <sup>2</sup> h | One-minute running average in 10-second steps.  |

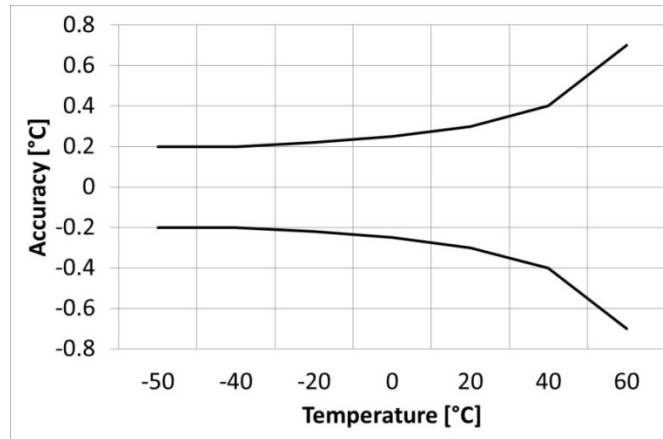


Figure 9. Accuracy over temperature range of the temperature sensor in the Vaisala weather station.

The tracker delivers a number of information about the location and operation of the tracker. When the data are stored in a common result file, it is possible to know exactly if the tracker has been operating as it is supposed to.

#### 4. Results from the new Climate station

The measurement program is made in Labview. The data are averaged of continuous recordings and read to a data file every minute. The data file is uploaded in a common directory at midnight and can be accessed the following day of the recordings.

The result file is described in Table 4. The result file contains measurements from:

- Module 1: NI9214 16-CH isothermal thermocouple input module
- Module 2: NI9214 16-CH isothermal thermocouple input module
- Module 3: NI9205 16-CH differential analog input module,
- Module 4: NI9870 4-Port RS232 serial module
- Module 5: N9217 4-CH RTD analog input module
- Sun tracker and sun sensor.

Table 4. Content of the output file

| Ch#   | Description  | Unit                    |
|---|--|-------------------------|
| Time(utc)   | UTC time: month, day, year, hour, minute, day<br>Danish winter time: +1 hour<br>Danish summer time: +2hour | [mm-dd-yyy<br>hh:mm:ss] |
| <b>Measurements from pyranometers and pyrhelimeter (Module 1-3)</b> |  |                         |
| Mod1Ch1   | CMP 11: Fractional horizontal diffuse irradiance. 1/8<br>Dome. Azimuth=39.5°                               | [W/m <sup>2</sup> ]     |
| Mod1Ch2   | CMP 11: Fractional horizontal diffuse irradiance. 1/16<br>Dome. Azimuth=39.5°                              | [W/m <sup>2</sup> ]     |
| Mod1Ch3   | CMP 11: Fractional horizontal diffuse irradiance. 1/8<br>Dome. Azimuth=84.5°                               | [W/m <sup>2</sup> ]     |
| Mod1Ch4   | CMP 11: Fractional horizontal diffuse irradiance. 1/16   | [W/m <sup>2</sup> ]     |

|          |   |                     |
|----------|---|---------------------|
|          | Dome. Azimuth=84.5°   |                     |
| Mod1Ch5  | CMP 11: Fractional horizontal diffuse irradiance. 1/8<br>Dome. Azimuth=129.5°   | [W/m <sup>2</sup> ] |
| Mod1Ch6  | CMP 11: Fractional horizontal diffuse irradiance. 1/16<br>Dome. Azimuth=129.5°  | [W/m <sup>2</sup> ] |
| Mod1Ch7  | CMP 11: Fractional horizontal diffuse irradiance. 1/8<br>Dome. Azimuth=174.5°   | [W/m <sup>2</sup> ] |
| Mod1Ch8  | CMP 11: Fractional horizontal diffuse irradiance. 1/16<br>Dome. Azimuth=174.5°  | [W/m <sup>2</sup> ] |
| Mod1Ch9  | CMP 11: Fractional horizontal diffuse irradiance. 1/8<br>Dome. Azimuth=-140.5°  | [W/m <sup>2</sup> ] |
| Mod1Ch10 | CMP 11: Fractional horizontal diffuse irradiance. 1/16<br>Dome. Azimuth=-140.5°   | [W/m <sup>2</sup> ] |
| Mod1Ch11 | CMP 11: Fractional horizontal diffuse irradiance. 1/8<br>Dome. Azimuth=-95.5°   | [W/m <sup>2</sup> ] |
| Mod1Ch12 | CMP 11: Fractional horizontal diffuse irradiance. 1/16<br>Dome. Azimuth=-95.5°  | [W/m <sup>2</sup> ] |
| Mod1Ch13 | CMP 11: Fractional horizontal diffuse irradiance. 1/8<br>Dome. Azimuth=-50.5°   | [W/m <sup>2</sup> ] |
| Mod1Ch14 | CMP 11: Fractional horizontal diffuse irradiance. 1/16<br>Dome. Azimuth=-50.5°  | [W/m <sup>2</sup> ] |
| Mod1Ch15 | CMP 11: Fractional horizontal diffuse irradiance. 1/8<br>Dome. Azimuth=-5.5°  | [W/m <sup>2</sup> ] |
| Mod1Ch16 | CMP 11: Fractional horizontal diffuse irradiance. 1/16<br>Dome. Azimuth=-5.5°   | [W/m <sup>2</sup> ] |
| Mod2Ch1  | Not in use  |                     |
| Mod2Ch2  | CM 11: Horizontal diffuse irradiance with shadow ring:<br>Radius=650 mm. Width=58 mm.   | [W/m <sup>2</sup> ] |
| Mod2Ch3  | CMP 11: Horizontal diffuse irradiance measured with<br>tracker.   | [W/m <sup>2</sup> ] |
| Mod2Ch4  | Not in use  |                     |
| Mod2Ch5  | CHP 1: Beam normal irradiance measured with tracker.<br>Internal instrument temperature measured with PT100<br>(see # 53)       | [W/m <sup>2</sup> ] |
| Mod2Ch6  | CM 11: Global irradiance  | [W/m <sup>2</sup> ] |
| Mod2Ch7  | CM 5: Total solar irradiance on 90° tilt West oriented  | [W/m <sup>2</sup> ] |
| Mod2Ch8  | CM 5: Total solar irradiance on 90° tilt North oriented   | [W/m <sup>2</sup> ] |
| Mod2Ch9  | CM 5: Total solar irradiance on 90° tilt East oriented.<br>Artificial horizon for rejection of ground reflected<br>irradiance.  | [W/m <sup>2</sup> ] |
| Mod2Ch10 | CM 5: Total solar irradiance on 90° tilt South oriented.<br>Artificial horizon for rejection of ground reflected<br>irradiance. | [W/m <sup>2</sup> ] |
| Mod2Ch11 | CM 5: Total solar irradiance on 45° tilt South oriented.  | [W/m <sup>2</sup> ] |
| Mod2Ch12 | Not in use  |                     |
| Mod2Ch13 | Not in use  |                     |
| Mod2Ch14 | Not in use  |                     |

|  |  |                           |
|--|--|---------------------------|
| Mod2Ch15   | Not in use   |                           |
| Mod2Ch16   | Not in use   |                           |
| Mod3Ch1  | Not in use   |                           |
| Mod3Ch2  | Not in use   |                           |
| Mod3Ch3  | Not in use   |                           |
| Mod3Ch4  | Not in use   |                           |
| Mod3Ch5  | Not in use   |                           |
| Mod3Ch6  | Not in use   |                           |
| Mod3Ch7  | Not in use   |                           |
| Mod3Ch8  | Not in use   |                           |
| Mod3Ch9  | Not in use   |                           |
| Mod3Ch10   | Not in use   |                           |
| Mod3Ch11   | Not in use   |                           |
| Mod3Ch12   | Not in use   |                           |
| Mod3Ch13   | Not in use   |                           |
| Mod3Ch14   | Not in use   |                           |
| Mod3Ch15   | Not in use   |                           |
| Mod3Ch16   | Not in use   |                           |
| <b>Measurements from Vaisala weather transmitter WXT520 (Module 4)</b> |  |                           |
| wind_dir_min   | Wind direction, minimum  | [°]                       |
| wind_dir_avg   | Wind direction, average  | [°]                       |
| wind_dir_max   | Wind direction, maximum  | [°]                       |
| wind_speed_min   | Wind speed, minimum  | [m/s]                     |
| wind_speed_avg   | Wind speed, average  | [m/s]                     |
| wind_speed_max   | Wind speed, maximum  | [m/s]                     |
| air_temperature  | Ambient air temperature  | [°C]                      |
| relative_humidity  | Relative humidity of ambient air   | [%]                       |
| air_pressure   | Ambient air pressure   | [Pa]                      |
| rain_accumulation  | Rain accumulation  | [mm]                      |
| rain_duration  | Rain duration  | [s]                       |
| rain_intensity   | Rain intensity   | [mm/h]                    |
| hail_accumulation  | Hail accumulation  | [hits/cm <sup>2</sup> ]   |
| hail_duration  | Hail duration  | [s]                       |
| hail_intensity   | Hail intensity   | [hits/cm <sup>2</sup> /h] |
| <b>Measurements from SPN 1 pyranometer (Module 4)</b>                  |  |                           |
| sunshine   | 0 if solar irradiance $\leq 300 \text{ W/m}^2$<br>1 if solar irradiance $> 300 \text{ W/m}^2$  | [-]                       |
| sun_total  | Total solar irradiance on horizontal with SPN1   | [W/m <sup>2</sup> ]       |
| sun_diffuse  | Diffuse solar irradiance on horizontal with SPN1   | [W/m <sup>2</sup> ]       |
| <b>Temperature measurements (Module 5)</b>                             |  |                           |
| RTD0_Pyrheliometer   | Pyrheliometer instrument internal temperature (see #21)<br>Should be used for temperature compensation:<br>Temperature [°C] ; deviation [%]: 50 40 30 20 10 0 -10 -20 ; 0.16 -0.02 -0.07 0.00 0.18 0.19 0.05 -0.48 | [°C]                      |
| RTD1   | Not in use   |                           |
| RTD2   | Not in use   |                           |
| RTD3_Cabinet   | Temperature in the cabinet of the measurement  | [°C]                      |

|   |   |                              |
|---|---|------------------------------|
|   | equipment   |                              |
| <b>Measurements/information from sun tracker SOLYS 2 and sun sensor</b> |   |                              |
| Azimuth_adjust  | Azimuth adjust of tracker by sun sensor                               | [°]                          |
| Zenith_adjust   | Zenith adjust of tracker by sun sensor                                | [°]                          |
| Azimuth   | Azimuth angle of the tracker/sun                                      | [°]                          |
| Zenith  | Zenith angle of the tracker/sun                                       | [°]                          |
| Function  | Function  |                              |
| Q1_Sun_intensity  | Direct normal solar irradiance on sun sensor, above_left              | [W/m <sup>2</sup> ]          |
| Q2_Sun_intensity  | Direct normal solar irradiance on sun sensor, below_left              | [W/m <sup>2</sup> ]          |
| Q3_Sun_intensity  | Direct normal solar irradiance on sun sensor, above_right             | [W/m <sup>2</sup> ]          |
| Q4_Sun_intensity  | Direct normal solar irradiance on sun sensor, below_right             | [W/m <sup>2</sup> ]          |
| Total_Sun_intensity   | Direct normal solar irradiance on sun sensor:<br>Q1+Q2+Q3+Q4          | [W/m <sup>2</sup> ]          |
| Solys_instrument_status   |   | [-]                          |
| Solys_gps_time  | GPS time from tracker: year, day, hour, minute, second,<br>milisecond | [yyyy ddd<br>hh mm ss<br>ms] |

## 5. References

- [1] Hans Lund, 1994. Solmålestationen. Rapport nr. 94-18. Juni 1994. Laboratoriet for Varmeisolering. Danmarks Tekninske Universitet.
- [2] Elsa Andersen<sup>a</sup>, Kristian Pagh Nielsen<sup>b</sup>, Janne Dragsted<sup>a</sup>, Simon Furbo<sup>a</sup>. Measurements of the angular distribution of diffuse irradiance. <sup>a</sup>Technical University of Denmark, Institute of Civil Engineering, Nordvej 119, 2800, Kgs. Lyngby, Denmark. <sup>b</sup>Danish Meterological Institute, Lyngbyvej 100, 2100 Copenhagen Ø, Denmark. In proceedings of International Conference on Solar Heating and Cooling for Buildings and Industry, SHC 2014.



**DTU Civil Engineering**  
**Department of Civil Engineering**  
Technical University of Denmark

Brovej, Building 118  
2800 Kgs. Lyngby  
Telephone 45 25 17 00

[www.byg.dtu.dk](http://www.byg.dtu.dk)

**ISBN 1601-8605**