



GEOMETRICAL CALIBRATION OF X-RAY CT SCANNERS

Stolfi, Alessandro; De Chiffre, Leonardo

Publication date:
2017

Document Version
Publisher's PDF, also known as Version of record

[Link back to DTU Orbit](#)

Citation (APA):
Stolfi, A., & De Chiffre, L. (2017). GEOMETRICAL CALIBRATION OF X-RAY CT SCANNERS. (Patent No. EP3195802).

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

(19)



(11)

EP 3 195 802 A1

(12)

EUROPEAN PATENT APPLICATION

(43) Date of publication:
26.07.2017 Bulletin 2017/30

(51) Int Cl:

A61B 6/03 (2006.01)	A61B 6/12 (2006.01)
A61B 6/00 (2006.01)	G06T 7/00 (2017.01)
G06T 7/60 (2017.01)	G01N 23/04 (2006.01)
G01B 21/04 (2006.01)	

(21) Application number: **16151878.2**

(22) Date of filing: **19.01.2016**

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME
Designated Validation States:
MA MD

(72) Inventors:

- **Stolfi, Alessandro**
2800 Kgs. Lyngby (DK)
- **De Chiffre, Leonardo**
2700 Brønshøj (DK)

(74) Representative: **Plougmann Vingtoft a/s**
Rued Langgaards Vej 8
2300 Copenhagen S (DK)

(71) Applicant: **Danmarks Tekniske Universitet**
2800 Kgs. Lyngby (DK)

(54) **GEOMETRICAL CALIBRATION OF X-RAY CT SCANNERS**

(57) A method of performing calibration scan and measurement scan in one and the same scanning operation with a calibration object having the fiducial marks arranged in positions spanning a volume enclosing at least a central portion of the measuring object. This avoids the need for one or more separate calibration scans to be performed in addition to the scanning of the measurement object. Considerable time is thereby saved. The fiducial objects are thus distributed, prefera-

bly evenly, around the measuring object, whereby homogeneous calibration is ensured. After having performed a scan of the measuring object together with the calibration object and thereby obtained scan data on the measuring object and corresponding scan data on the calibration object the scan data on the fiducial marks of the calibration object are used to calibrate the CT scanner, and the scan data on the measuring object are used to calculate geometric properties of the measuring object.

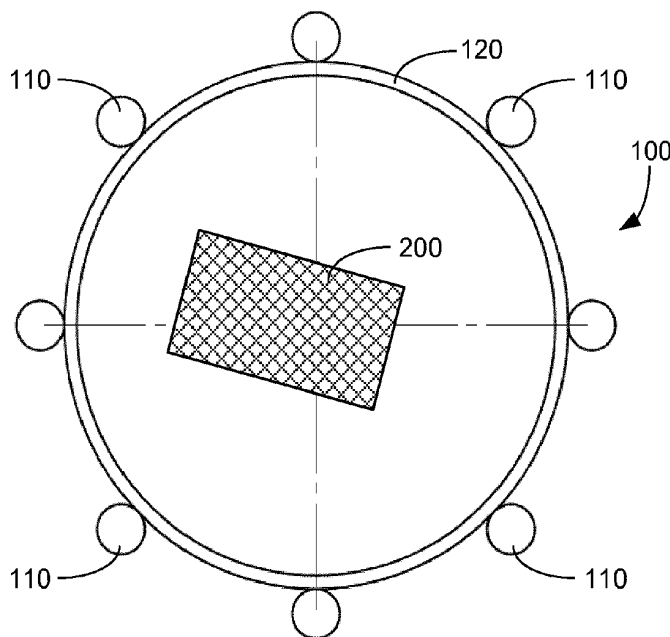


Fig. 2

EP 3 195 802 A1

Description

FIELD OF THE INVENTION

[0001] The invention relates to geometrical calibration of X-ray CT scanners in general and in particular to geometrical calibration of industrial X-ray CT scanners used in the field of dimensional metrology. Typical areas of use of CT in industry are in the detection of flaws such as voids and cracks and particle analysis in materials. In metrology CT allows measuring the external as well as the internal geometry of complex products. Thus, CT metrology can be used for nondestructive measurement of external and internal geometries.

BACKGROUND OF THE INVENTION

[0002] Industrial CT scanners used in metrology provide high resolution in the order of micrometres. The procedure of measuring a measuring object in three dimensions is time consuming. Furthermore, to ensure accurate and reliable measuring results, the scanners need to be calibrated using a calibration object with precisely known geometry, typically involving physical elements such as spheres, which is also time consuming. In critical and demanding cases calibration is performed both before and after scanning the measuring object. The entire procedure including pre-calibration, scanning the measuring object and post calibration may last several hours.

[0003] It is therefore desirable to reduce the time for CT scanning a measuring object including the time for calibrating the CT scanner.

SUMMARY OF THE INVENTION

[0004] The invention provides a method of performing calibration scan and measurement scan in one and the same scanning operation with a calibration object having the physical elements defining fiducial marks arranged in positions spanning a volume enclosing at least a central portion of the measuring object. This avoids the need for one or more separate calibration scans to be performed in addition to the scanning of the measurement object. Obviously, considerable time is thereby saved.

[0005] The fiducial marks are thus distributed around the measuring object, whereby homogeneous calibration is ensured. It is preferred that the volume spanned by the fiducial marks encloses the entire measuring object and not only a central portion.

[0006] In a preferred embodiment the calibration object comprises an X-ray transmissive tubular or ring-shaped supporting structure with the fiducial marks arranged in fixed positions on a surface of the supporting structure. Advantageously, the tubular or ring-shaped supporting structure includes a rigid base-element fixed to an end of the supporting structure.

[0007] In another preferred embodiment the calibration object comprises a rigid base with a plurality of X-ray

transmissive elongate supporting elements extending from the base with the fiducial marks fixed to the supporting elements. This allows portions of the measuring object to extend through spaces between the supporting elements and outside the volume spanned by the fiducial marks.

[0008] An X-ray transmissive support can be used to support the measuring object to ensure that the measuring object, or at least a central portion of it, is within the volume spanned by the fiducial marks.

[0009] After having performed a scan of the measuring object together with the calibration object and thereby obtained scan data on the measuring object and corresponding scan data on the calibration object the scan data on the fiducial marks of the calibration object are used to calibrate the CT scanner, and the scan data on the measuring object are used to calculate geometric properties of the measuring object.

BRIEF DESCRIPTION OF THE DRAWINGS

[0010]

Figure 1 shows a side view of a tubular calibration object according to the invention;

Figure 2 shows a view in the axial direction of the tubular calibration object in figure 1;

Figure 3 shows a side view of another calibration object according to the invention; and

Figure 4 shows a view in the axial direction of the calibration object in figure 4;

DETAILED DESCRIPTION OF THE INVENTION

[0011] In figures 1 and 2 is shown a calibration object 100 with a plurality of possible positions for fiducial marks 110 secured to the outer surface of a tubular supporting structure 120 in precisely known positions relative to each other. Preferably, fiducial marks 110 should not be in positions on the calibration object where, at any time during scanning, a line through two or more of the fiducial marks will intersect the focal point of the X-ray source. This reduces the risk of image artefacts. The tubular supporting structure 120 is made of a rigid material with low X-ray absorption, such as carbon-fiber reinforced polymer, whereby image artefacts caused by X-ray absorption in the tubular supporting structure 120 are minimised. The fiducial marks 110 are preferably spherical elements with identical diameters and an X-ray transmissivity which matches that of the measuring object. Thus, when the measuring object is of a material with a relatively low X-ray transmissivity such as a polymer material, ruby is a preferred material for the fiducial marks 110. The tubular supporting structure 120 has a base 130 preferably with a stepped diameter fixed to one end of the tubular supporting structure 120 to further increase the mechanical stability of the calibration object 100. Preferred materials for the base include INVAR, which is a nickel-iron

alloy notable for its uniquely low coefficient of thermal expansion, and carbon fibre reinforced polymer. The calibration object 100 as a whole as well as each of its components has high mechanical and thermal stability. In the shown example the tubular supporting structure 120 is in the shape of a circular cylinder, but other configurations are possible such as a polyhedron or a portion of a sphere. Figure 2 shows a measuring object 200 placed within the calibration object 100.

[0012] In figures 3 and 4 is shown another calibration object with four fiducial marks 310 arranged in precisely known positions relative to each other so that the fiducial marks define three linearly independent vectors, i.e. they are not included in the same plane. The calibration object 300 comprises a rigid base 330, preferably made of INVAR, with a plurality of X-ray transmissive elongate supporting elements 320 extending from the base with the fiducial marks 310 fixed to the supporting elements. A preferred material for the supporting elements 320 is carbon-fiber-reinforced polymer. Each of the supporting elements 320 can have one or more fiducial marks 310 fixed thereto, e.g. at an end as shown or at the side. A measuring object 200 placed within a volume spanned by the fiducial marks 310 of the calibration object 300. Advantageously, an X-ray transmissive support 340 is used to support the measuring object.

or ring-shaped supporting structure (120) includes a rigid base-element (130) fixed to an end of the supporting structure (120).

- 5 4. A method according to claim 1 wherein the calibration object (300) comprises a rigid base (330) with a plurality of X-ray transmissive elongate supporting elements (320) extending from the base (330) with the fiducial marks (310) fixed to the supporting elements (320).
- 10 5. A method according to any one of the preceding claims wherein an X-ray transmissive support (340) is used to support the measuring object.
- 15 6. A method according to any one of the preceding claims wherein the scan data on the fiducial marks of the calibration object (100, 300) are used to calibrate the CT scanner.
- 20 7. A method according to any one of the preceding claims wherein the scan data on the measuring object (200) are used to calculate geometric properties of the measuring object (200).
- 25

Claims

- 30 1. A method of measuring three dimensional dimensions of a measuring object (200) using an X-ray CT scanner having a measuring volume, the method comprising
arranging the measuring object (200) together with
a calibration object (100, 300) in the measuring volume;
scanning the measuring object (200) and the calibration object (100, 300) together in the measuring volume so as to obtain scan data on the measuring
object (200) and corresponding scan data on the calibration object (100, 300); wherein
the calibration object (100, 300) has at least four fiducial marks (110, 310) arranged in known positions relative to each other, the fiducial marks (110, 310)
defining at least three linearly independent vectors, and
the fiducial marks (110, 310) are arranged in positions spanning a volume enclosing at least a central portion of the measuring object (200).
50
- 55 2. A method according to claim 1 wherein the calibration object (100) comprises an X-ray transmissive tubular or ring-shaped supporting structure (120) with the fiducial marks (110) arranged in fixed positions on a surface of the supporting structure (120).
3. A method according to claim 2 wherein the tubular

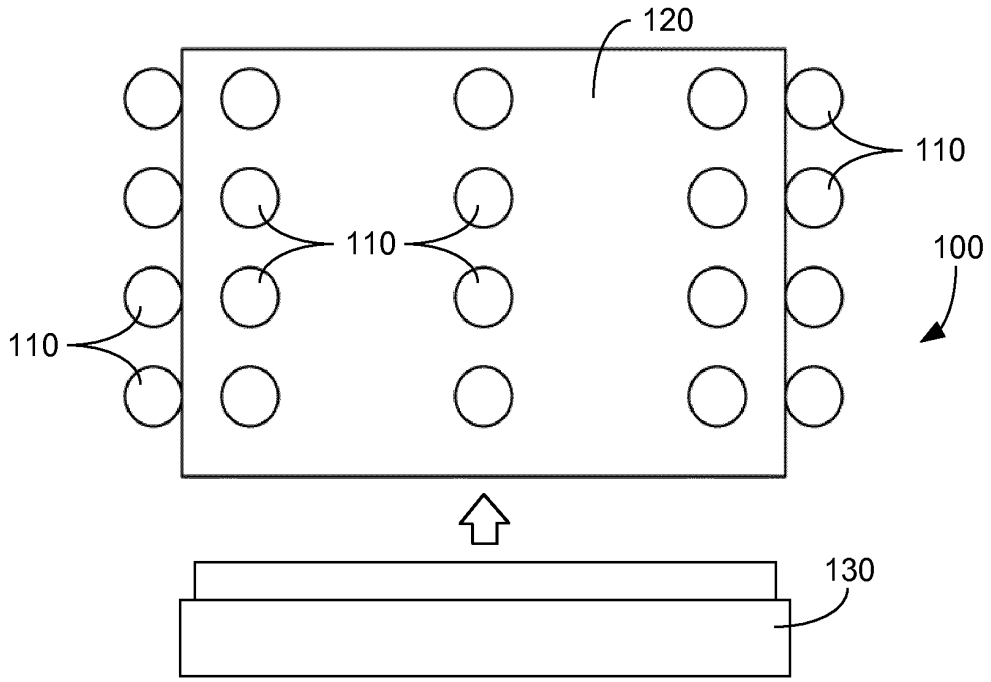


Fig. 1

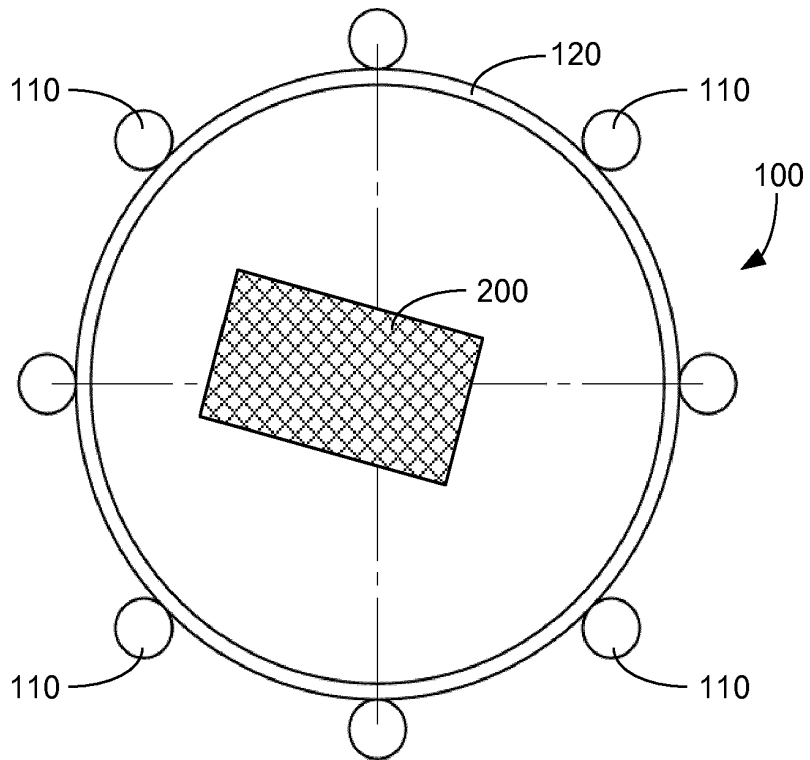


Fig. 2

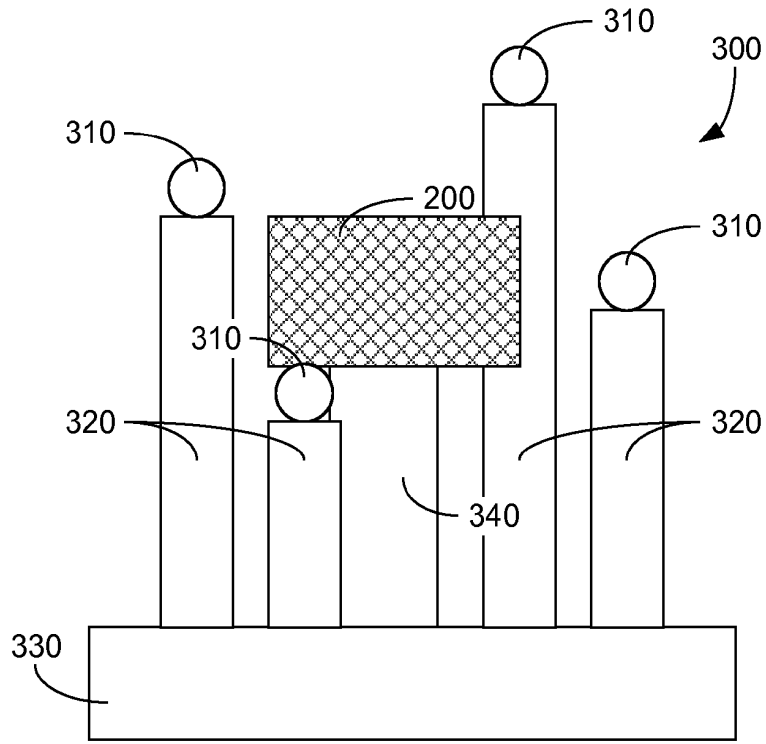


Fig. 3

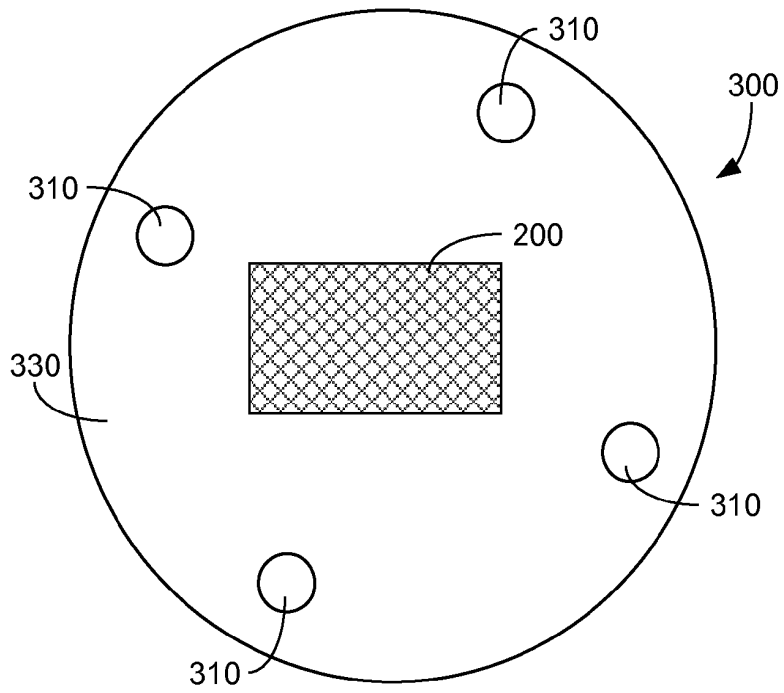


Fig. 4



EUROPEAN SEARCH REPORT

Application Number
EP 16 15 1878

5

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	JP 2014 190933 A (GUNMA PREFECTURE) 6 October 2014 (2014-10-06) * paragraph [0005] - paragraph [0024]; claims 1-6; figures 1-6 * -----	1,2,6,7	INV. A61B6/03 A61B6/12 A61B6/00 G06T7/00
X	WO 2014/154627 A1 (NIKON METROLOGY NV) 2 October 2014 (2014-10-02) * page 9, line 12 - line 21 * * page 11, line 31 - line 36; figure 10 * * page 16, line 1 - line 14 * * page 16, line 25 - line 34 * * page 20, line 19 - page 22, line 3 * * page 23, line 35 - page 24, line 15 * -----	1-7	G06T7/60 G01N23/04 G01B21/04
X	NORBERT K. STROBEL: "Improving 3D image quality of x-ray C-arm imaging systems by using properly designed pose determination systems for calibrating the projection geometry", PROCEEDINGS OF SPIE, vol. 5030, 1 January 2003 (2003-01-01), pages 943-954, XP055008635, ISSN: 0277-786X, DOI: 10.1117/12.479945 * Section 2.2 and legends of figs. 2 and 3; figure 2 * -----	1-3,5-7	TECHNICAL FIELDS SEARCHED (IPC) A61B G06T G01N G01B
X	US 2005/117708 A1 (CHO YOUNG-BIN [CA] ET AL) 2 June 2005 (2005-06-02) * paragraph [0113]; figures 2,16 * * paragraph [0124] - paragraph [0125] * ----- -/--	1-3,5-7	
The present search report has been drawn up for all claims			
Place of search Munich		Date of completion of the search 3 June 2016	Examiner Martinez Möller, A
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	

EPO FORM 1503 03.82 (P04/C01)

10

15

20

25

30

35

40

45

50

55



EUROPEAN SEARCH REPORT

Application Number
EP 16 15 1878

5

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
A	KRUTH J P ET AL: "Computed tomography for dimensional metrology", CIRP ANNALS, vol. 60, no. 2, 2011, pages 821-842, XP028262022, ISSN: 0007-8506, DOI: 10.1016/J.CIRP.2011.05.006 [retrieved on 2011-06-03] * Section 7. 3 in p. 832-833 & section 7.7 in p. 835-837.; figure 29 * -----	1-7	
			TECHNICAL FIELDS SEARCHED (IPC)
The present search report has been drawn up for all claims			
Place of search Munich		Date of completion of the search 3 June 2016	Examiner Martinez Möller, A
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	

10

15

20

25

30

35

40

45

1

EPO FORM 1503 03.02 (P04C01)

50

55

ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.

EP 16 15 1878

5

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

03-06-2016

10

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
JP 2014190933 A	06-10-2014	NONE	
WO 2014154627 A1	02-10-2014	GB 2512714 A	08-10-2014
		US 2016030133 A1	04-02-2016
		WO 2014154627 A1	02-10-2014
US 2005117708 A1	02-06-2005	EP 1654516 A1	10-05-2006
		US 2005117708 A1	02-06-2005
		WO 2005015125 A1	17-02-2005

15

20

25

30

35

40

45

50

55

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82